

# User Manual: Pediatric Plates and Screws used for Bone Fixation: An Engineering Reference Dataset

## Tool Reference

**RST Reference Number:** RST24PD01.1

**Date of Publication:** 10/23/2024

**Recommended Citation:** U.S. Food and Drug Administration. (2024). *Pediatric Plates and Screws used for Bone Fixation: An Engineering Reference Dataset* (RST24PD01.1). <https://cdrh-rst.fda.gov/pediatric-plates-and-screws-used-bone-fixation-engineering-reference-dataset>

**Overview**

Engineering characteristics of bone fixation plate and screws (HRS and/or HWC product codes) were collected from premarket notification submissions cleared in FDA’s 510(k) database<sup>1</sup>. The search was limited to medical devices with metallic, non-absorbable implants only and at least one pediatric age group<sup>2,3</sup> listed in the cleared indications for use. Spinal, maxillofacial, and cranial devices were excluded. Approximately 250 510(k) submissions met these criteria between 1976 and 2024. From there, submissions with the greatest number of device components were selected to help represent the widest range of pediatric-specific characteristics; this resulted in recording information from 24 submissions cleared between 2000 and 2024. To maintain confidentiality, all information collected from the 510(k) database was aggregated and de-identified with nominal values across multiple submissions presented instead of exact dimensions. After collating the collected data, the device characteristics were compared for consistency against anthropometric data of pediatric anatomy from published literature.<sup>4,5</sup>

The engineering characteristics are applicable to the following types of bones: tibia, fibula, femur, pelvis, metacarpals, carpals, metatarsals, tarsals, humerus, ulna, radius, calcaneus, clavicle, pelvis, olecranon, scapula, acetabulum, phalanges.

**Engineering Characteristics of Pediatric Bone Fixation Plates and Screws**

Pediatric bone fixation plates and screws were found to have the engineering characteristics outlined in Table 1 and Table 2, respectively. Generic geometric drawings of the plates can be found in Figure 1.

<b>Table 1: Engineering Characteristics of Pediatric Bone Fixation Plates</b>
Plate Material: Titanium alloys, Cobalt Chromium alloys, Stainless Steel <sup>6-12</sup>
Plate Length (L): 16 - 400mm
Plate Shaft Width (W <sub>s</sub> ): 7.0 - 15.5mm
Plate Head Width (W <sub>h</sub> ): 7.0 - 38mm
Plate Thickness (T): 1.0 - 5mm
Plate Hole Diameter (D <sub>h</sub> , widest point if tapered): 1.5 – 7.5mm
Number of Holes, Long Axis: 2 – 30 with or without hole threading
Plate Blade Angle: 0-50 degrees
Plate Geometries (note: definitions are found in ASTM F382 and ASTM F384 <sup>9-10</sup> or are self-explanatory): straight, contour, angled, tubular, letter-shaped (S, T, Y), cloverleaf, cobra head

<b>Table 2: Engineering Characteristics of Pediatric Bone Fixation Screws</b>
Screw Material: Titanium alloys, Cobalt Chromium alloys, Stainless Steel <sup>6-12</sup>
Screw Length: 5 - 150mm
Screw Head Diameter (at widest point if tapered): 1.5 - 7.5mm
Screw Head Depth: 0.8 - 4 mm
Major thread diameter: 1.5 - 7mm
Screw Geometries (note: definitions are found in ASTM F543 <sup>11</sup> ): cancellous, cortical, non-tapping, partially threaded, self-tapping, types HA/HB/HC/HD, compression (with and without head)

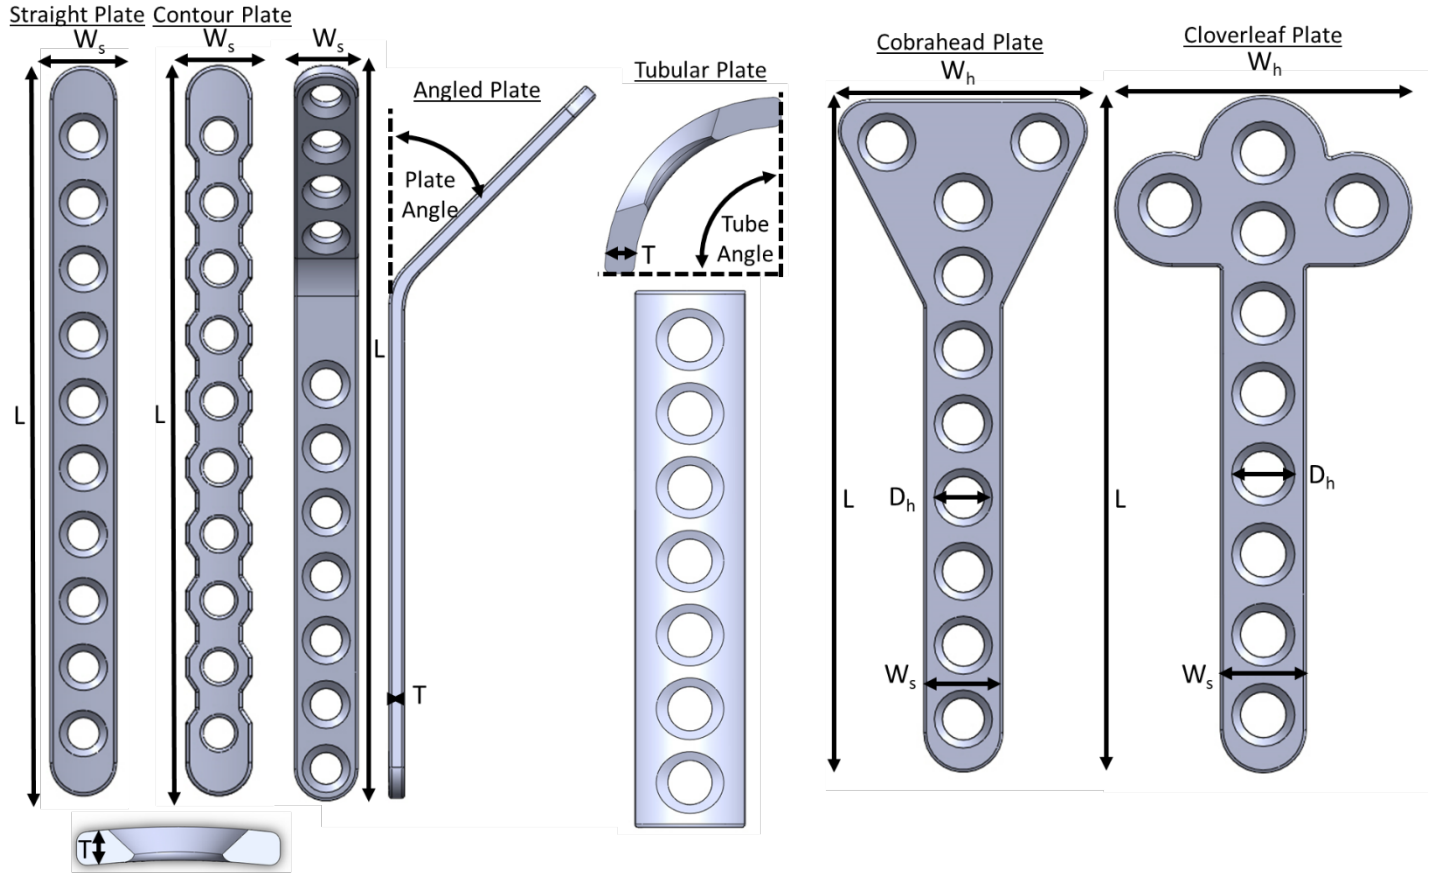


Figure 1: Example plate geometries based on definitions found in ASTM 382-17 and ASTM 384-17<sup>8,9</sup>. Plate Geometries (Left to Right): Straight Plate, Contour Plate, Angled Plate, Tubular Plate, Cobrahead Plate, Cloverleaf Plate. Geometries are labeled with defined dimensions.  $W_s$ : Shaft width,  $W_h$ : Head width,  $L$ : Overall Length,  $T$ : Thickness,  $D_h$ : Hole Diameter

## References:

1. Food and Drug Administration. *510(k) Premarket Notification*.  
<https://www.accessdata.fda.gov/scripts/cdrh/cfdocs/cfpmn/pmn.cfm>
2. Code of Federal Regulations [21 CFR 814.3(s)]
3. Premarket Assessment of Pediatric Medical Devices: Guidance for Industry and Food and Drug Administration Staff. March 14, 2014. <https://www.fda.gov/media/73510/download>
4. Pietak, A., Ma, S., Beck, C. W., & Stringer, M. D. (2013). Fundamental ratios and logarithmic periodicity in human limb bones. *J Anat*, 222(5), 526-537. <https://doi.org/10.1111/joa.12041>
5. McDowell, M. A., Fryar, C. D., Ogden, C. L., & Flegal, K. M. (2008). Anthropometric reference data for children and adults: United States, 2003-2006. *Natl Health Stat Report*(10), 1-48.  
<https://www.ncbi.nlm.nih.gov/pubmed/25585443>
6. ASTM Standard F136-13(2021)e1, "Standard Specification for Wrought Titanium-6Aluminum-4Vanadium ELI (Extra Low Interstitial) Alloy for Surgical Implant Applications (UNS R56401)" ASTM International, West Conshohocken, PA, 2019, DOI: 10.1520/F0136-13R21E01, [www.astm.org](http://www.astm.org)
7. ASTM Standard F138-19, "Standard Specification for Wrought 18Chromium-14Nickel-2.5Molybdenum Stainless Steel Bar and Wire for Surgical Implants (UNS S31673)" ASTM International, West Conshohocken, PA, 2019, DOI: 10.1520/F0138-19, [www.astm.org](http://www.astm.org)
8. ASTM Standard F139-19, "Standard Specification for Wrought 18Chromium-14Nickel-2.5Molybdenum Stainless Steel Sheet and Strip for Surgical Implants (UNS S31673)" ASTM International, West Conshohocken, PA, 2019, DOI: 10.1520/F0139-19, [www.astm.org](http://www.astm.org)
9. ASTM Standard F382-17, "Standard Specification and Test Method for Metallic Bone Plates" ASTM International, West Conshohocken, PA, 2017, DOI: 10.1520/F0382-17, [www.astm.org](http://www.astm.org)
10. ASTM Standard F384-17, "Standard Specifications and Test Methods for Metallic Angled Orthopedic Fracture Fixation Devices" ASTM International, West Conshohocken, PA, 2017, DOI: 10.1520/F0384-17, [www.astm.org](http://www.astm.org)
11. ASTM Standard F543-17, "Standard Specification and Test Methods for Metallic Medical Bone Screws" ASTM International, West Conshohocken, PA, 2017, DOI: 10.1520/F0543-17, [www.astm.org](http://www.astm.org)
12. ASTM Standard F2229-21, "Standard Specification for Wrought, Nitrogen Strengthened 23Manganese-21Chromium-1Molybdenum Low-Nickel Stainless Steel Alloy Bar and Wire for Surgical Implants (UNS S29108)" ASTM International, West Conshohocken, PA, 2017, DOI: 10.1520/F0543-17, [www.astm.org](http://www.astm.org)